

The background of the advertisement is a close-up, artistic shot of water splashing or flowing, creating a series of interconnected, translucent, and shimmering droplets and streams. The entire scene is bathed in a vibrant, monochromatic green light, which gives the water a glowing, ethereal quality. The droplets vary in size and focus, with some in sharp foreground and others blurred in the background, creating a sense of depth and movement.

AURACLE™ LINE

Professional
Bio-Regeneration

AURA
AESTHETICS

Professional Education Disclaimer

This document is intended exclusively for qualified healthcare professionals for scientific and educational discussion. It is not intended as a consumer advertisement, product label, or public promotional material. The products described herein may be registered or notified as cosmetic products in certain jurisdictions and must be used strictly in accordance with the approved local classification, label, instructions for use, and applicable regulations. Any off-label, invasive, injectable, or procedure-based use is the sole responsibility of the treating healthcare professional and must only be considered where permitted by local laws, professional standards, institutional policies, and patient consent requirements. CSN Pharma and Aura Aesthetics do not promote unauthorized injectable use of cosmetic products.

AURACLE

The Science of Skin Bio-Regeneration

Skin aging is a progressive decline in repair capacity, extracellular matrix quality, hydration balance, barrier function and tissue resilience.

- **AURACLE %2** focuses on repair-first regeneration using a pure PDRN strategy.
- **AURACLE PLUS** focuses on visible skin quality enhancement using Polynucleotides, Hyaluronic Acid, biomimetic peptides, tone-supportive ingredients and collagen-supportive components.

Both products are designed for professional treatment planning, not volumization. Product choice should be based on the dominant skin concern, edema risk, pigmentation tendency, skin barrier status, and previous aesthetic procedure history.

AURACLE **LINE**



From Cellular Repair to Advanced Skin Regeneration

Polynucleotides and PDRN are DNA-derived bioactive molecules used in regenerative aesthetic concepts. They are valued for their role in supporting tissue repair pathways, extracellular matrix quality, hydration balance and visible skin resilience.

Their clinical performance depends on concentration, formulation design, treatment interval, patient selection and physician expertise.

Structural Comparison




FEATURE	PN	PDRN
<ul style="list-style-type: none"> • Molecular structure • Molecular weight • Skin quality role • Clinical concept 	<ul style="list-style-type: none"> • Longer-chain DNA fragments • Higher (sustained activity) • Elasticity, hydration and dermal quality • Sustained bio-regeneration support • Skin revitalization and firmness 	<ul style="list-style-type: none"> • Shorter-chain DNA fragments • Lower (faster diffusion) • Repair, recovery and tissue support • Repair-focused regeneration support

Common Biological Actions

PN - PDRN

Benefits & Mechanisms

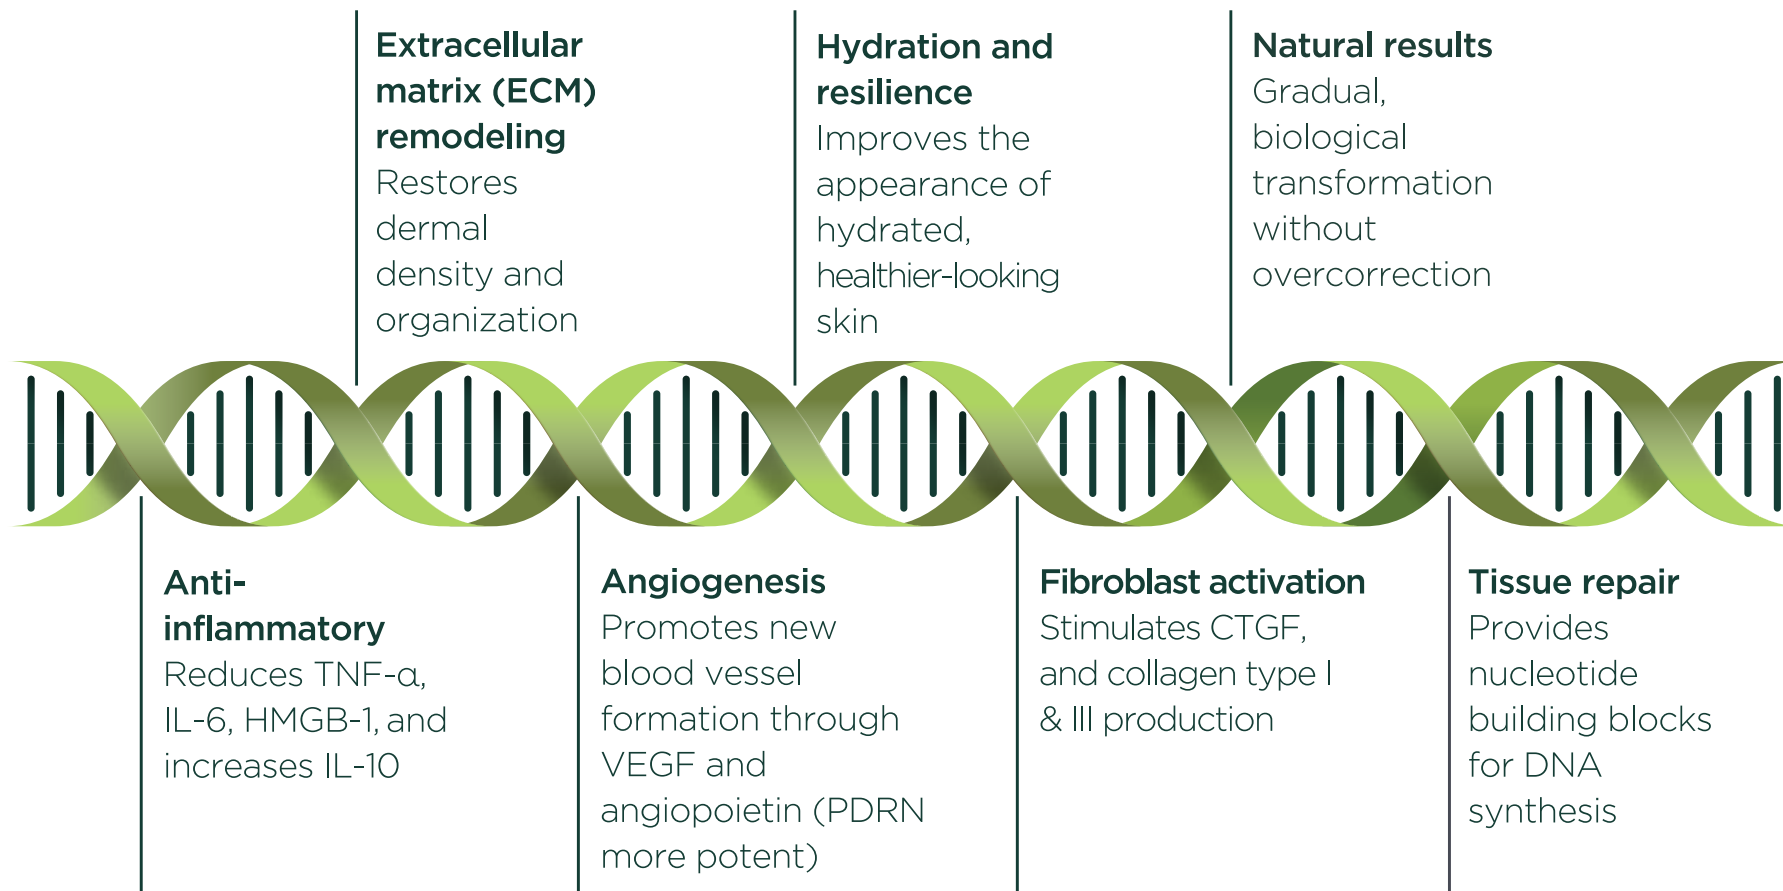

AURACLE 2%

Pure PDRN Bio-Repair

A sterile, isotonic, phosphate-buffered PDRN formulation designed to support cellular skin repair, skin integrity and recovery-focused skin quality enhancement.

Best for: repair, recovery, stressed skin, early aging, post-procedure recovery support and skin integrity.



Indications:

- Dull and stressed skin
- Early signs of aging
- Skin barrier impairment
- Thin or fragile skin
- Mild texture irregularity
- Post-procedure recovery




Ingredients:

- Polydeoxyribonucleotide: 40 mg
- Lidocaine HCl
- Phosphate buffer pH 7 q.s.



Syringe:

2 x 2 ml

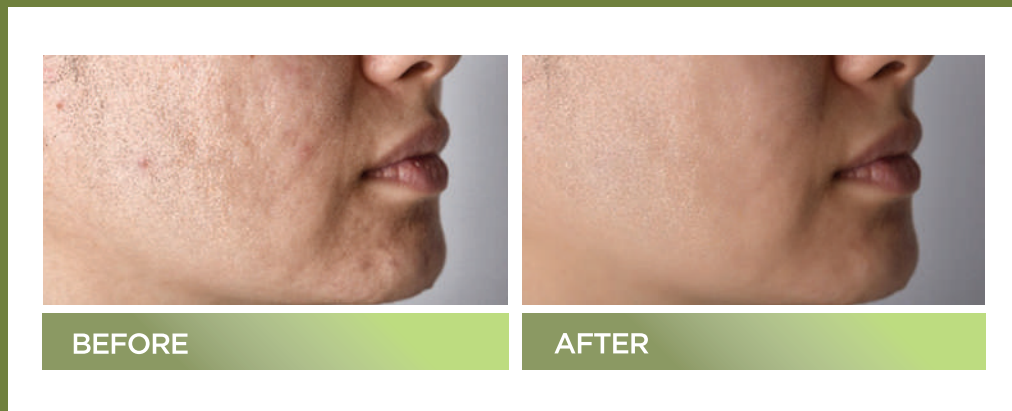

• TARGET LAYER

Dermis

• TECHNIQUE

Superficial intradermal micro droplet,
0.02-0.05 mL per point, ~1 cm spacing


• AREA

Full face, neck, décolletage, dorsal hands

• INTERVAL

Initial: 3 sessions, every 2-3 weeks

Maintenance: every 4-6 months if required

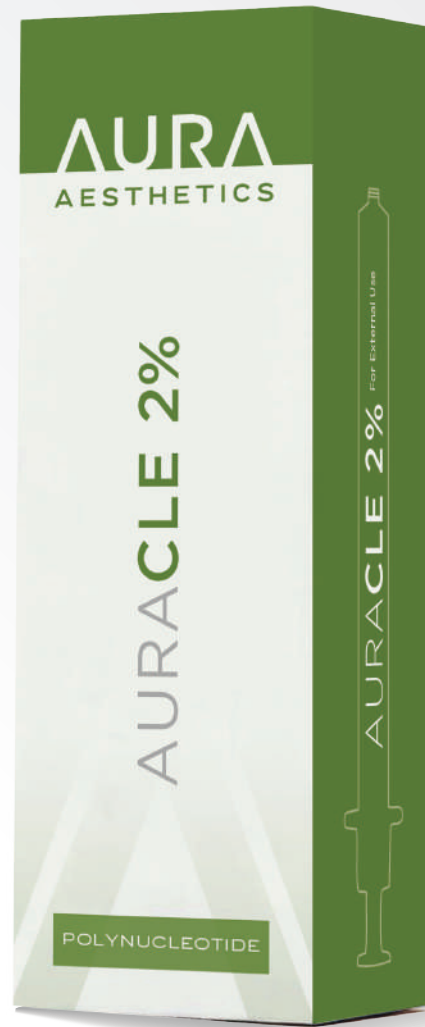

AURACLE PLUS

Multi-Functional Bio-Regeneration Complex

A multi-functional bio-regeneration complex combining PN, hyaluronic acid, biomimetic peptides, collagen-supportive components and tone-supportive ingredients to improve hydration, radiance, elasticity, fine-line appearance and overall skin quality.

Best for: hydration, radiance, uneven tone, fine lines, dullness and multi-dimensional revitalization.



Indications:

- Dehydrated skin
- Uneven tone appearance
- Loss of brightness and radiance
- Enlarged pores, irregular texture
- Fine lines




Ingredients:

- Sodium hyaluronate
- Polynucleotide (PN)
- Tranexamic acid
- Niacinamide
- Glutathione
- Peptide complex
- Recombinant collagen III
- Lidocaine HCl
- Phosphate buffer G1/2



Syringe:

2 x 2 ml

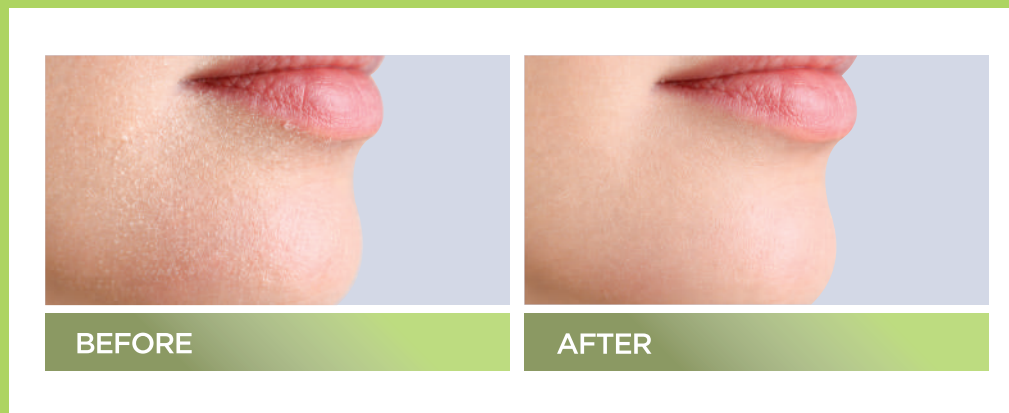

• TARGET LAYER

Papillary dermis

• TECHNIQUE

Superficial intradermal multi-point injection, 0.02-0.05 mL per point, ~1 cm spacing

• AREA

Full face, neck, décolletage, dorsal hands

• INTERVAL

Initial: 2 sessions, 4 weeks interval


Maintenance: every 4-6 months if required




Product Selection Algorithm

When should I use each product?

STEP 1 ASSESS SKIN CONDITION

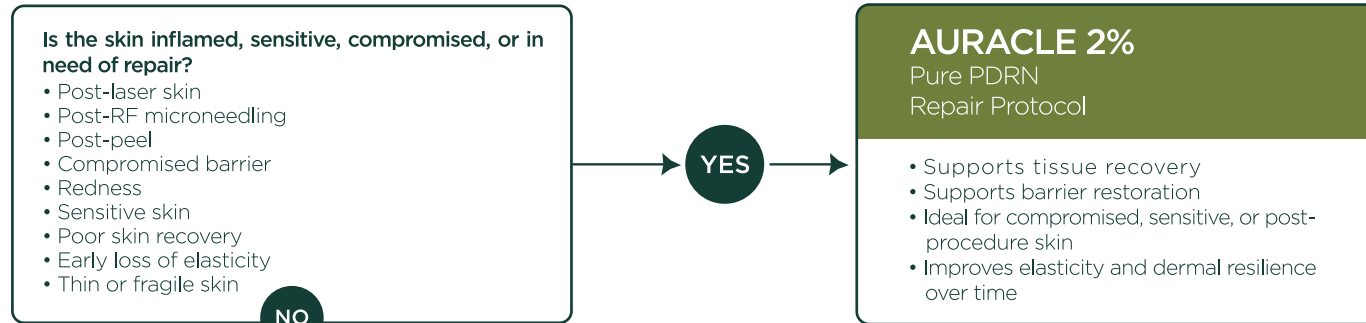

STEP 2 ASSESS QUALITY CONCERNS

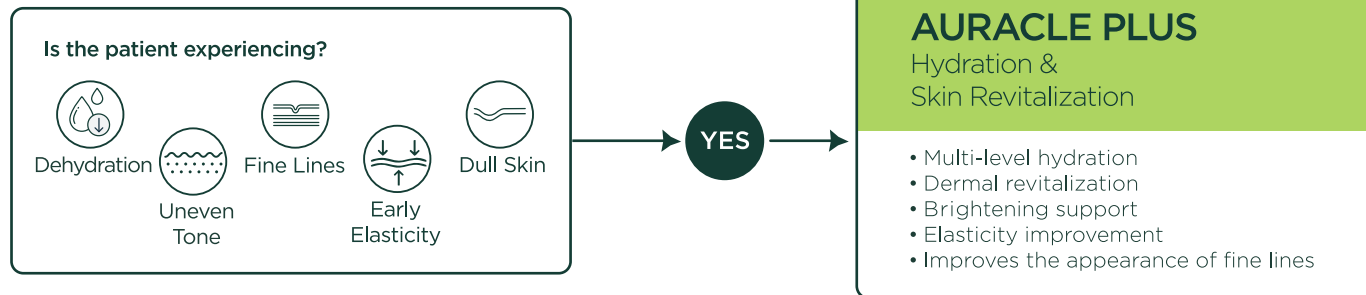

Optional AuraFamily Add-Ons

Add only after selecting the core AURACLE pathway.
Use according to indication, anatomy, tissue response and treatment intensity.

AURASOME

Exosome Supports
Recovery, glow, biological skin support.

Every 3 weeks according to indication.

AURACLE NAD+

ReGen / Boost
Cellular energy, tired-looking skin, slow recovery.

ReGen: 2-4 weeks after core.
Boost: 4-6 months.

AURAFEEL

Volume & Contour
Structural correction; AURACLE improves skin quality.

Same day different zones or 1-2 weeks same area.

AURACTURA

Collagen Stimulation
Laxity and dermal support.

Usually, 2-4 weeks apart from AURACLE.

RITUALAURA

Homecare Maintenance
Barrier, hydration, photoprotection and maintenance.

Daily protocol.

Combination Protocol & Treatment Timeline

When should I combine products?

<p>REPAIR PROTOCOL</p>	<p>Ideal patient:</p> <ul style="list-style-type: none"> • Sensitive • Inflamed • Post-procedure • Compromised skin 	<p>WEEK 0 AURACLE 2%</p> <p>WEEK 2-3 AURACLE 2%</p> <p>WEEK 4-6 AURACLE 2%</p>	<p>MAINTENANCE Every 4-6 months</p>
<p>HYDRATION & SKIN QUALITY PROTOCOL</p>	<p>Ideal patient:</p> <ul style="list-style-type: none"> • Dehydration • Fine lines • Dullness 	<p>WEEK 0 AURACLE PLUS</p> <p>WEEK 3-4 AURACLE PLUS</p> <p>WEEK 6-8 AURACLE PLUS If needed</p>	<p>MAINTENANCE Every 4-6 months</p>
<p>REPAIR + HYDRATION COMBINATION PROTOCOL</p>	<p>Ideal patient:</p> <ul style="list-style-type: none"> • Fragile • Dehydrated skin • Post-procedure 	<p>WEEK 0 AURACLE 2%</p> <p>WEEK 3-4 AURACLE PLUS</p> <p>WEEK 6-8 REASSESS AURACLE 2% or AURACLE PLUS Based on dominant residual concern</p>	<p>MAINTENANCE Every 4-6 months</p>



TIMING
Optimal intervals for best results



PERSONALIZED
Adapted to individual skin biology



SYNERGISTIC
Maximizing the power of each product



SCIENTIFIC
Evidence-based regenerative approach

CLINICAL TRIAL SUMMARY

Evaluation of safety and efficacy of AURACLE 2% for improvement of facial skin elasticity and rejuvenation

DESIGN & METHODS

• STUDY	• Phase II, multicenter
• PRODUCT	• AURACLE 2% - PDRN 40 mg / 2mL
• PARTICIPANTS	• 20 adults with facial aging
• PROTOCOL	• 2 intradermal sessions
• INTERVAL	• 4 weeks apart
• VISIT	• Baseline + Week 8


INVESTIGATOR GAIS

Significant improvement was observed in




of participants at week 8 by blinded investigator GAIS assessment.

OBJECTIVE CUTOMETRY

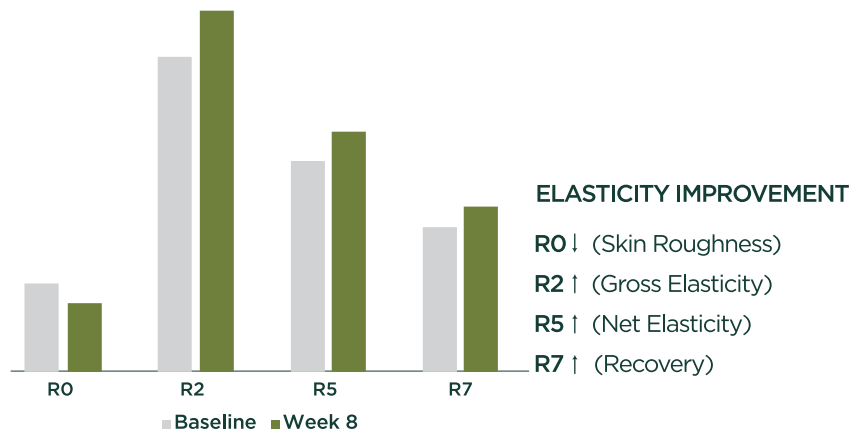

PARTICIPANT REPORTED OUTCOME

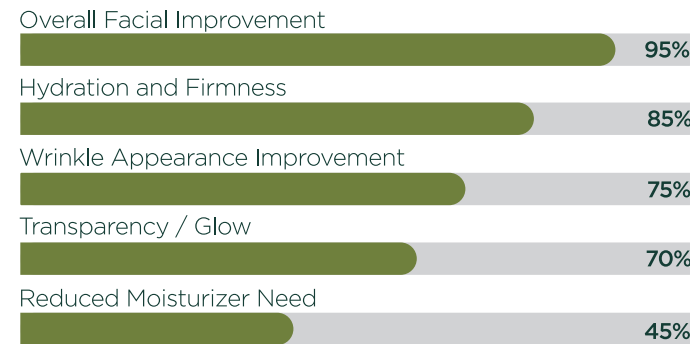

Safety & Tolerability

- No serious adverse events
- Expected local reactions
- Transient redness/swelling/papules

AURACLE™ LINE

FROM CELL TO SURFACE

- > Advanced bio-regenerative solutions
- > Designed for skin restoration
- > Predictable rejuvenation outcomes



Contact us at:
+1 604 544 5958

1641 Welch Street,
North Vancouver, BC, V7P 3G9 Canada

aurafamily.co.com

AURA